

The Helios Range

EvapoSensor & EvapoMeter

-  Use for irrigation scheduling - saves water
-  Measures Evaporation-Transpiration
-  Outputs in Degree Days which relates to water use by the crop
-  Wet & dry black 'leaf' elements react to RH, T, wind and radiation
-  Compares very well with AWS PET calculations

This sensor and meter system was produced by Skye Instruments during their participation in the HortLink project "Improving the Efficiency of Water Use in Container-Grown Nursery Stock", however it is suitable for use in any horticulture or agriculture application.

The Skye EvapoSensor consists of 2 black 'leaf' elements, one dry and one kept wet via a wick and a water reservoir. The temperature of these 2 'leaves' are measured individually and the



temperature differential is accumulated and stored by the EvapoMeter over time.

The design of the EvapoSensor was initialised by Horticulture Research International at East Malling, Kent, UK. The 2 simulated leaves are affected by their local environment just like plant leaves, and react to the four weather factors which drives water loss from plants, namely relative humidity, air temperature, wind speed and solar radiation.

Comparisons of the EvapoSensor directly against Potential Evaporation-Transpiration calculations, made using the Penman-Monteith method from automatic weather station measurements, are extremely

good, please see overleaf for details.

The HortLink project showed that scheduling irrigation with the EvapoMeter reduced total water use while maintaining crop quality.

The EvapoSensor can be used with most dataloggers or controllers, including the Skye DataHog logger. Alternatively the specially designed EvapoMeter will record and display temperature differentials in Day Degree totals of 24 hour periods and cumulative totals.

The advantage of the EvapoMeter is that the display can be easily read daily by technical and non-technical staff alike, connection to a PC is not necessary.



SPECIFICATIONS Meter


Housing	Dimensions	Weight	Sensor Connector	Display	Controls	Operating Temperature	Measurement Temperature	Resolution
Grey ABS base with clear lid. Sealed to IP65	122 x 120 x 55mm	450 grams including magnet	Binder sub-miniature 3 pin socket, sealed to IP65 when mated with plug or blanking cap	16 x 2 line alphanumeric liquid crystal display	2 magnetically operated reed switches to activate display menus	-20 to +70°C	-55 to +125°C	0.0625°C
Accuracy	Measurement Frequency	Memory	Alarm Feature	Calibration feature	Power	Power Consumption	Clock	Inputs
Typically better than 0.2°C at 25°C. Total error of 0.5°C over the range -55 to +85°C	Every 1 minute	Stores 4 parameters:- Total Accumulated Degree Hours since last reset (maximum 4095.9 before rollover). Previous Total Accumulated Degree Hours. Accumulated Degree Hours in current 24 hour period. Total Accumulated Degree Hours in previous 24 hour period. Memory is not lost if main battery fails	Flashing red LED if Degree Hour threshold is met or exceeded	To normalise differences between a sensor pair	PP3 or MN1604 9 volt alkaline battery. Typical battery life 6.5 weeks. Display of battery voltage and status indication. LED display switches off if inactive for 10 seconds to conserve power	'Sleeping' mode with green LED flashing - 360µA. 'Sleeping' mode with green LED and red alarm LED flashing - 600µA	24 hour real time clock, backed up by a separate lithium battery if main battery fails	Two temperature inputs from a single SKTS 500D/I EvapoMeter

PET COMPARISON

Two EvapoSensors were installed in an outdoor site, one at a crop canopy height so that it would be subject to irrigation with the crop, and the second at 1m above the canopy and sprinklers. An automatic weather station was also installed nearby and Potential Evaporation-Transpiration (PET) calculated from measurements of relative humidity, air temperature, wind speed and solar radiation using the Penman-Monteith method.

The graph shows excellent correlation between the pair of EvapoSensors, irrespective of whether in the irrigation zone or not, and also between the weather station PET calculations.

Reference: More for the Pots. Article in The Grower Magazine, p 14 & 15, issue March 14 2002.

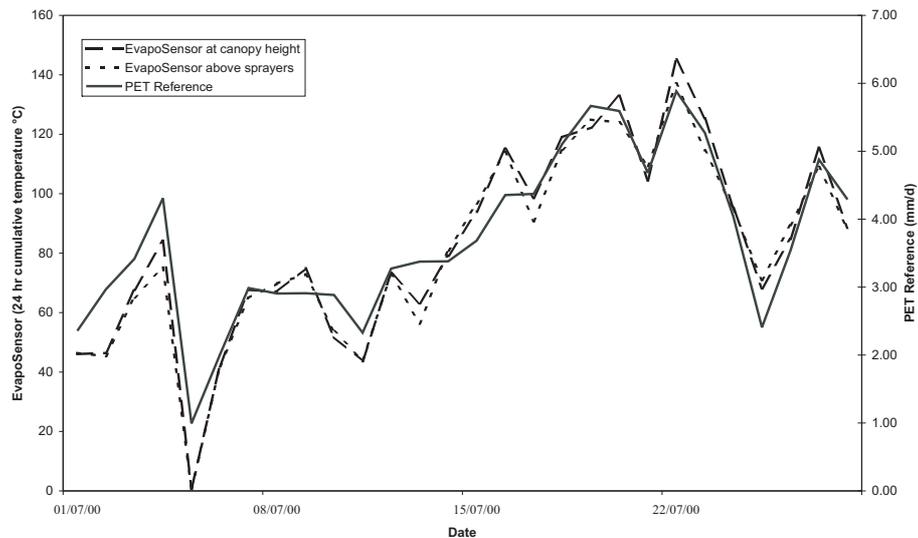

ORDERING INFORMATION

EvapoSensor
SKTS 500/D/I

EvapoSensor with connector for EvapoMeter

Meter
SEM 550

EvapoMeter with Display

Skye Instruments Ltd

21, Ddole Enterprise Park
Llandrindod Wells
Powys LD1 6DF
United Kingdom

TEL +44 (0)1597 824811

FAX +44 (0)1597 824812

EMAIL skyeemail@skyeinstruments.com

WEB <http://www.skyeinstruments.com>

